

流式细胞术检测T细胞表面受体




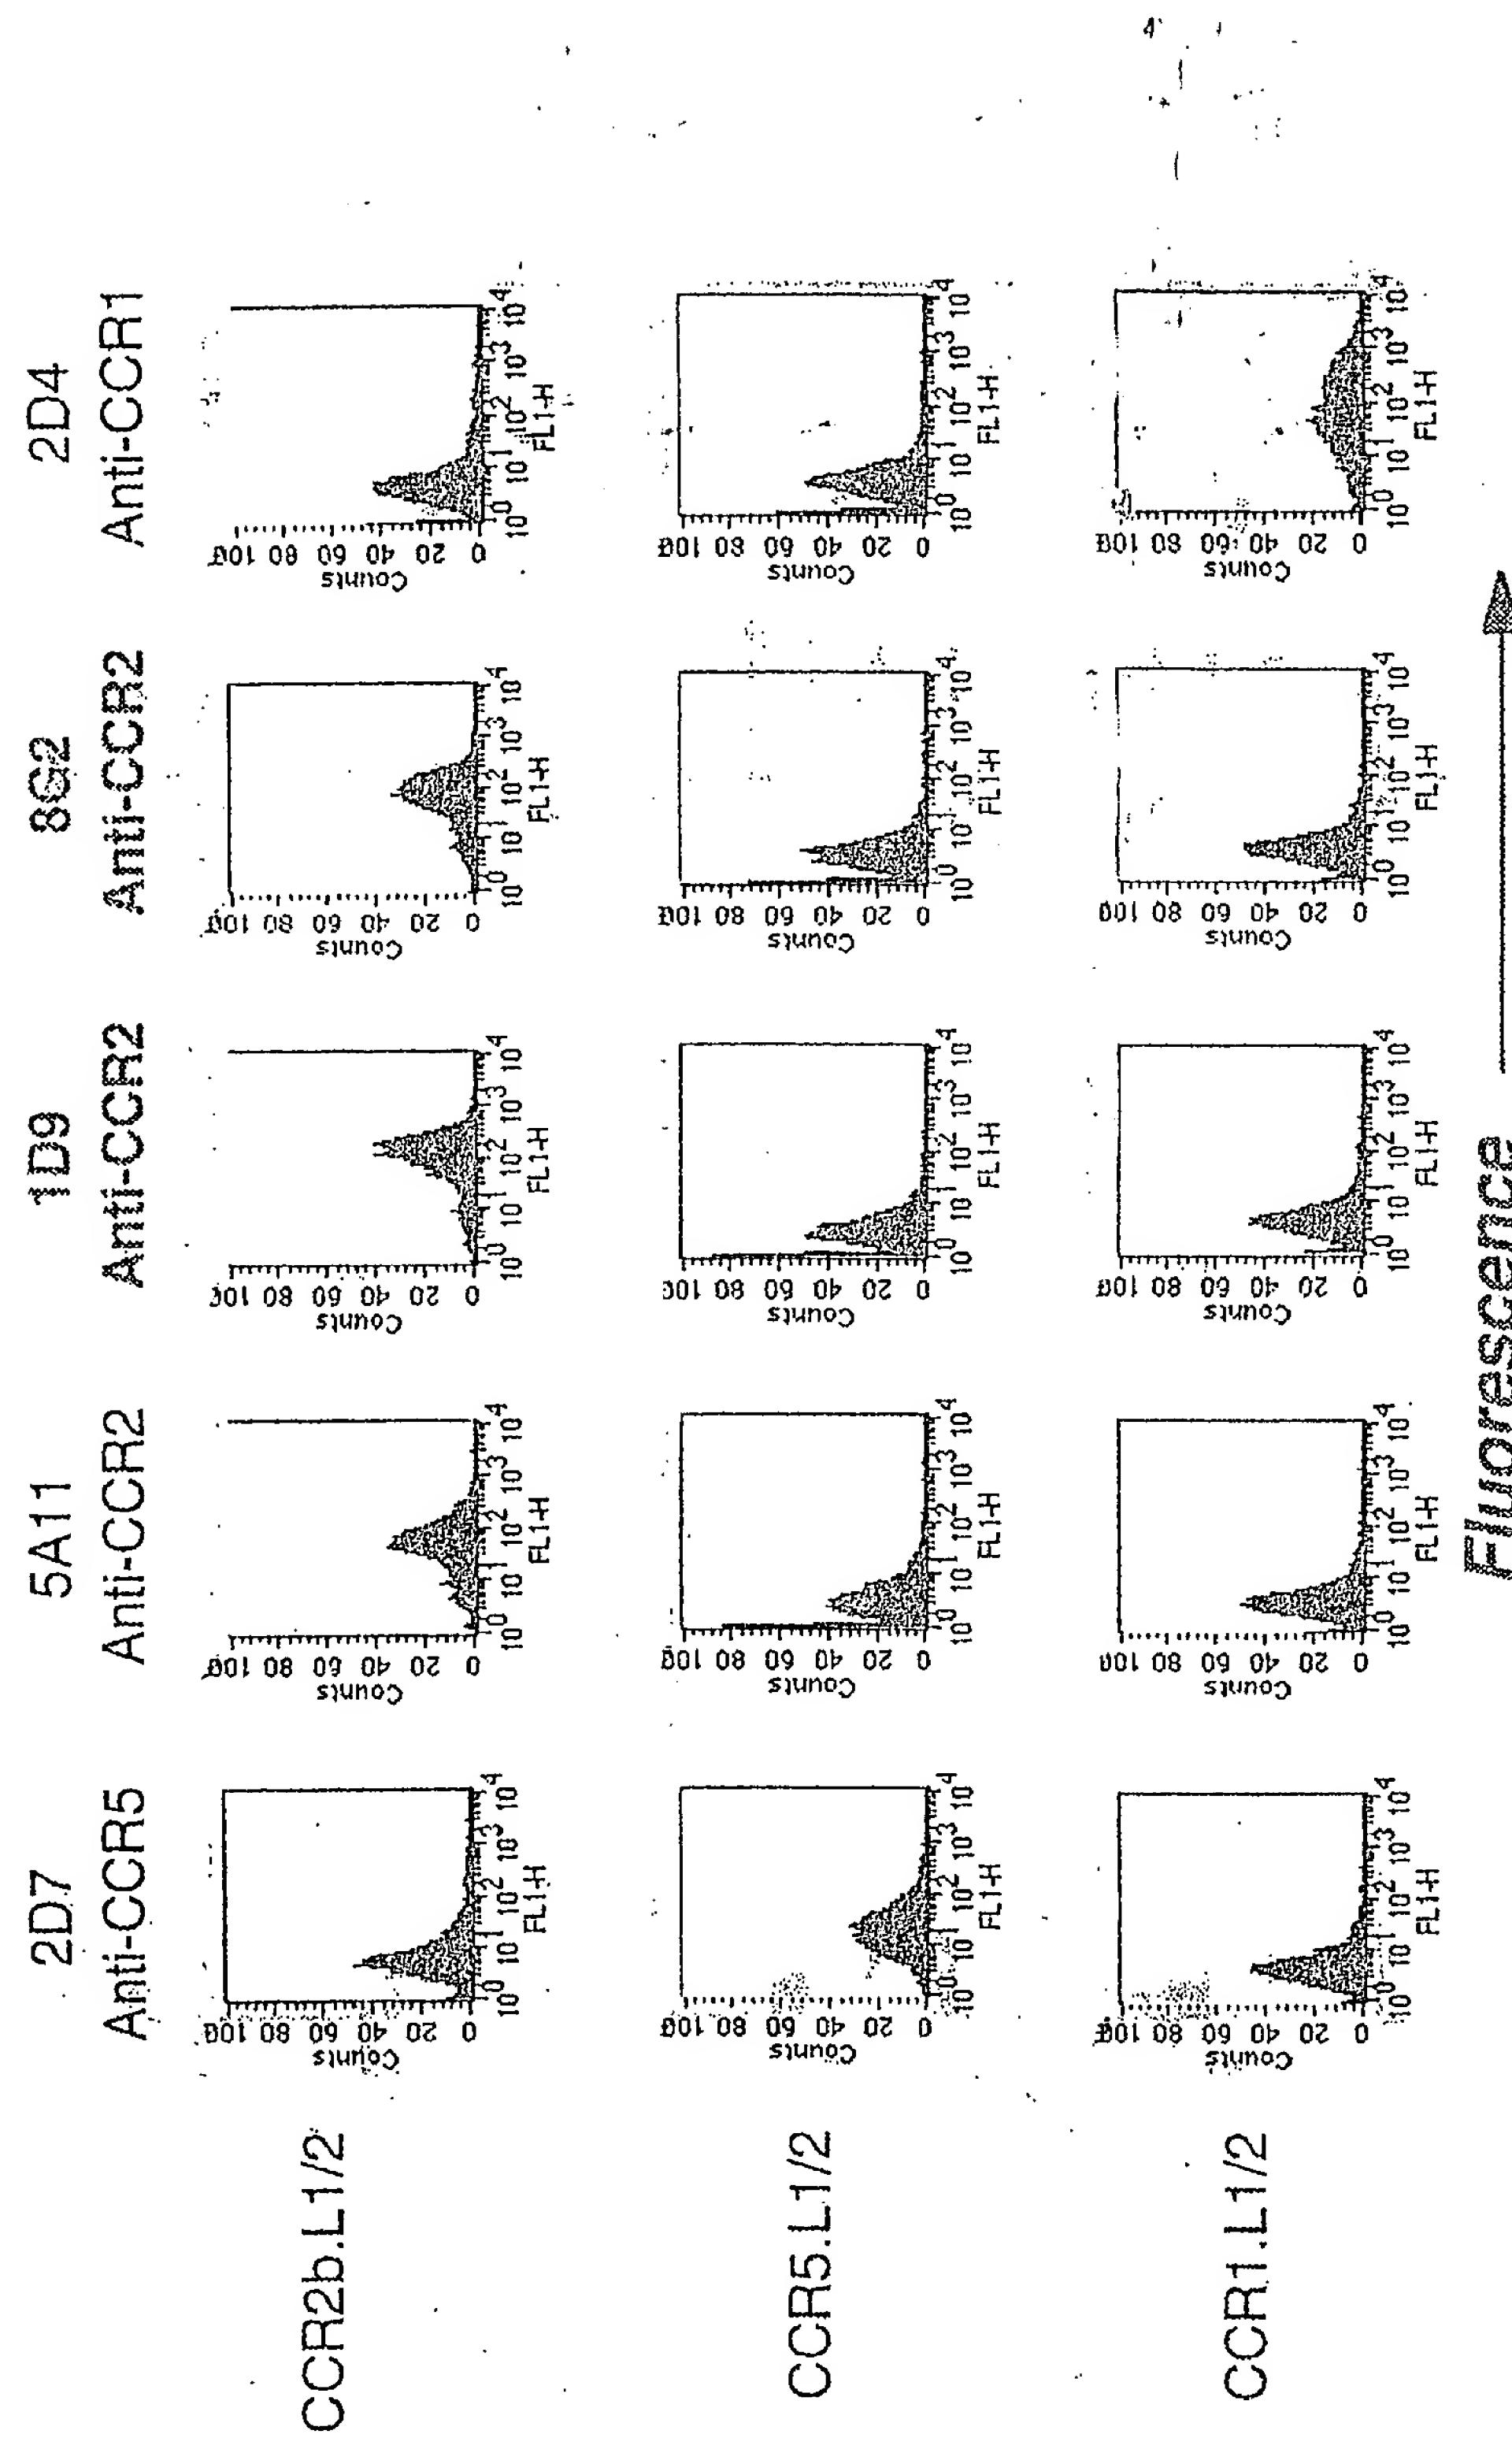



FIG. 1

Forward Scatter


Monocytes

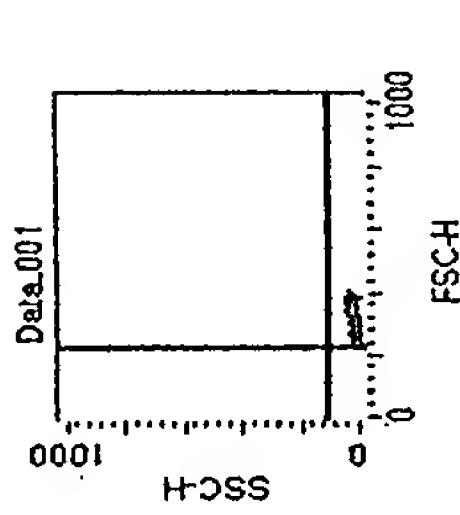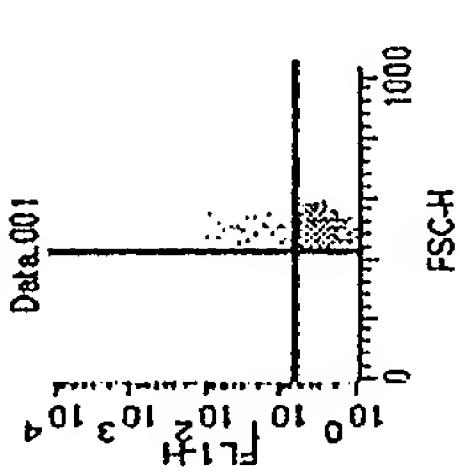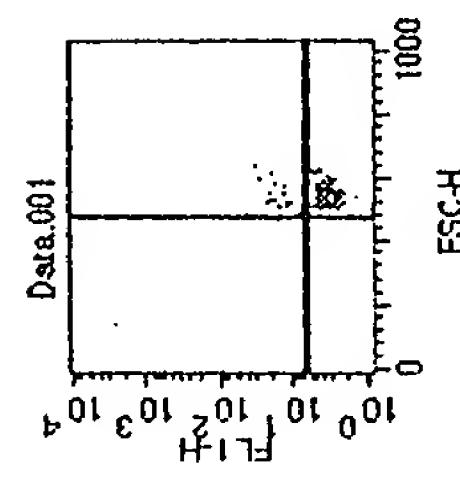

Granulocytes

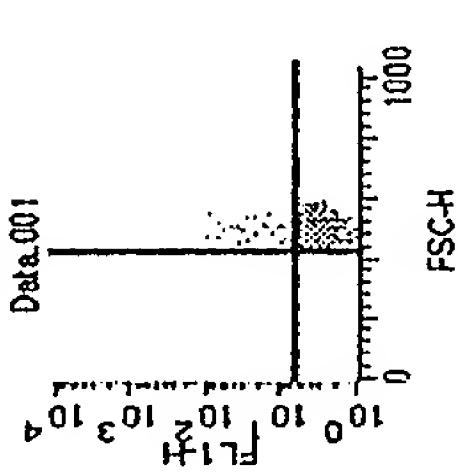

Lymphocytes

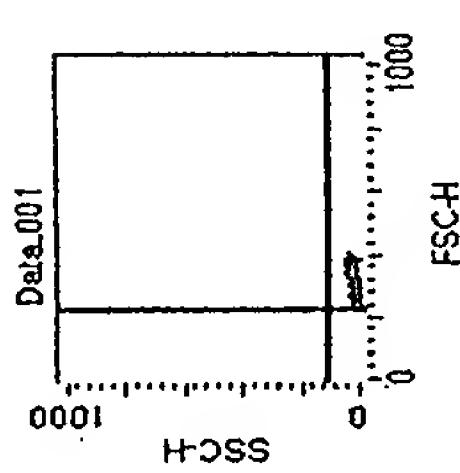

PBS

5A11

1D9

8G2

Fluorescence

FIG. 2

Forward Scatter

FIGURE THREE


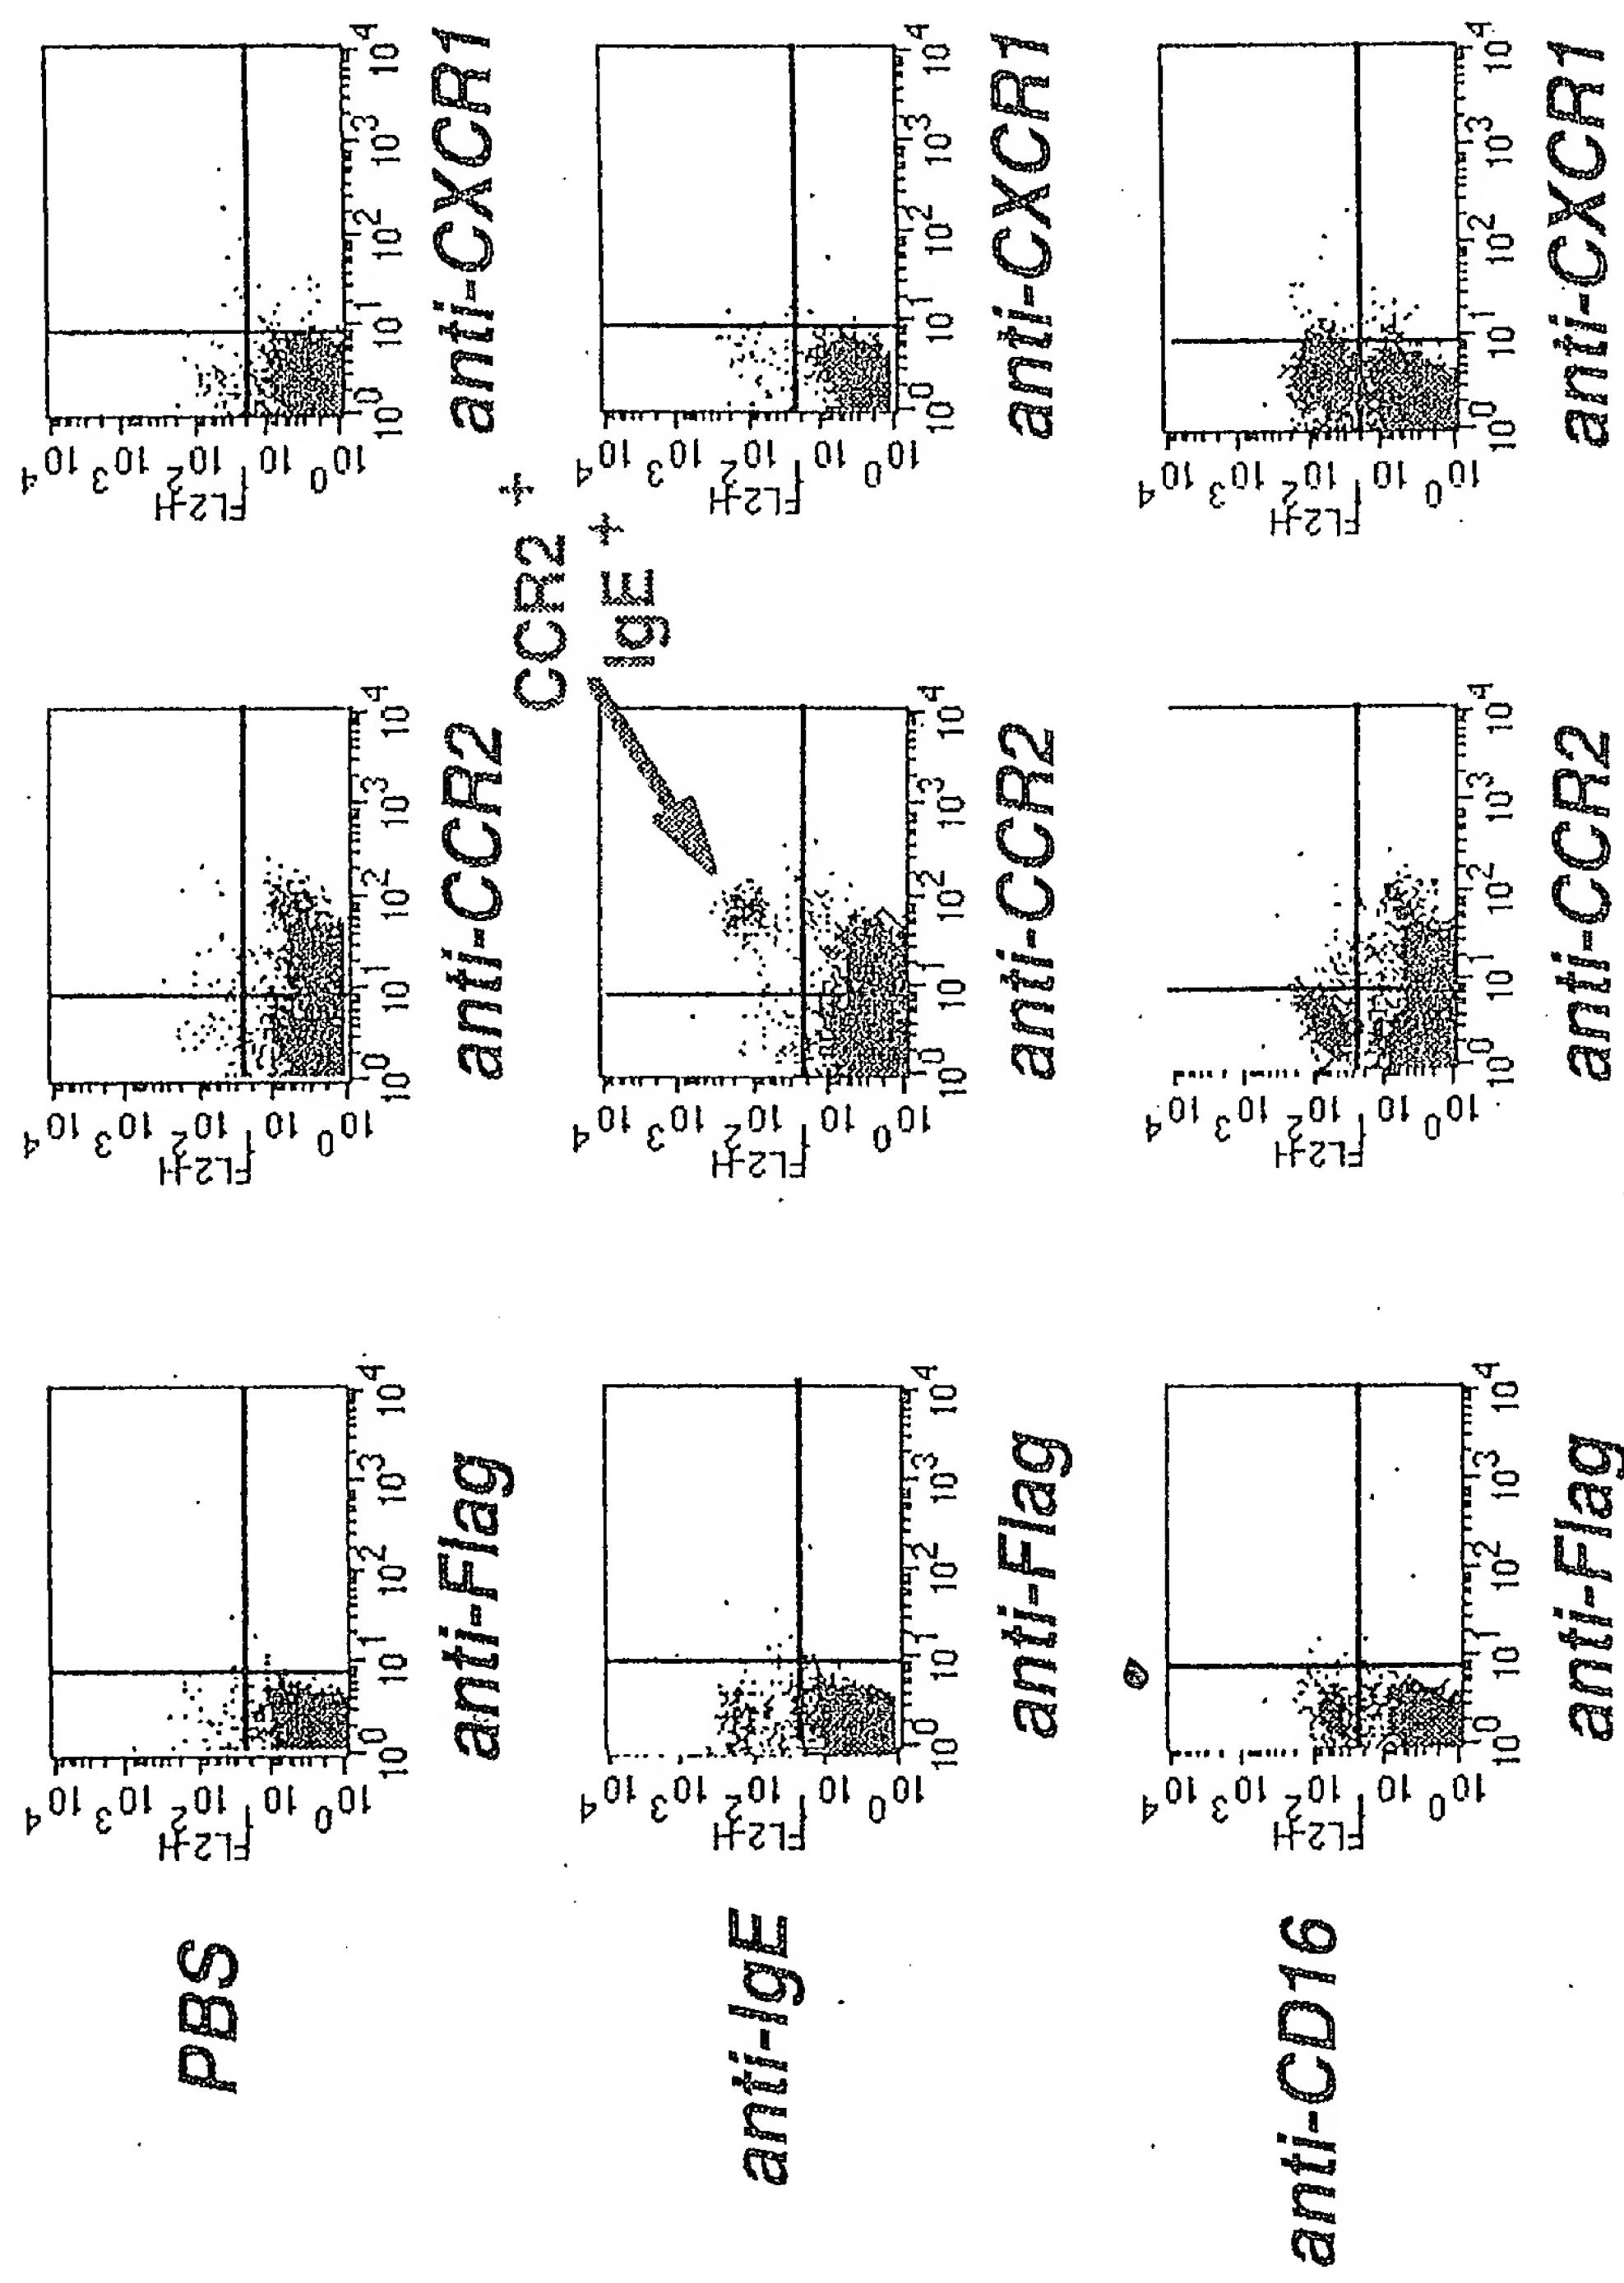


FIG. 3

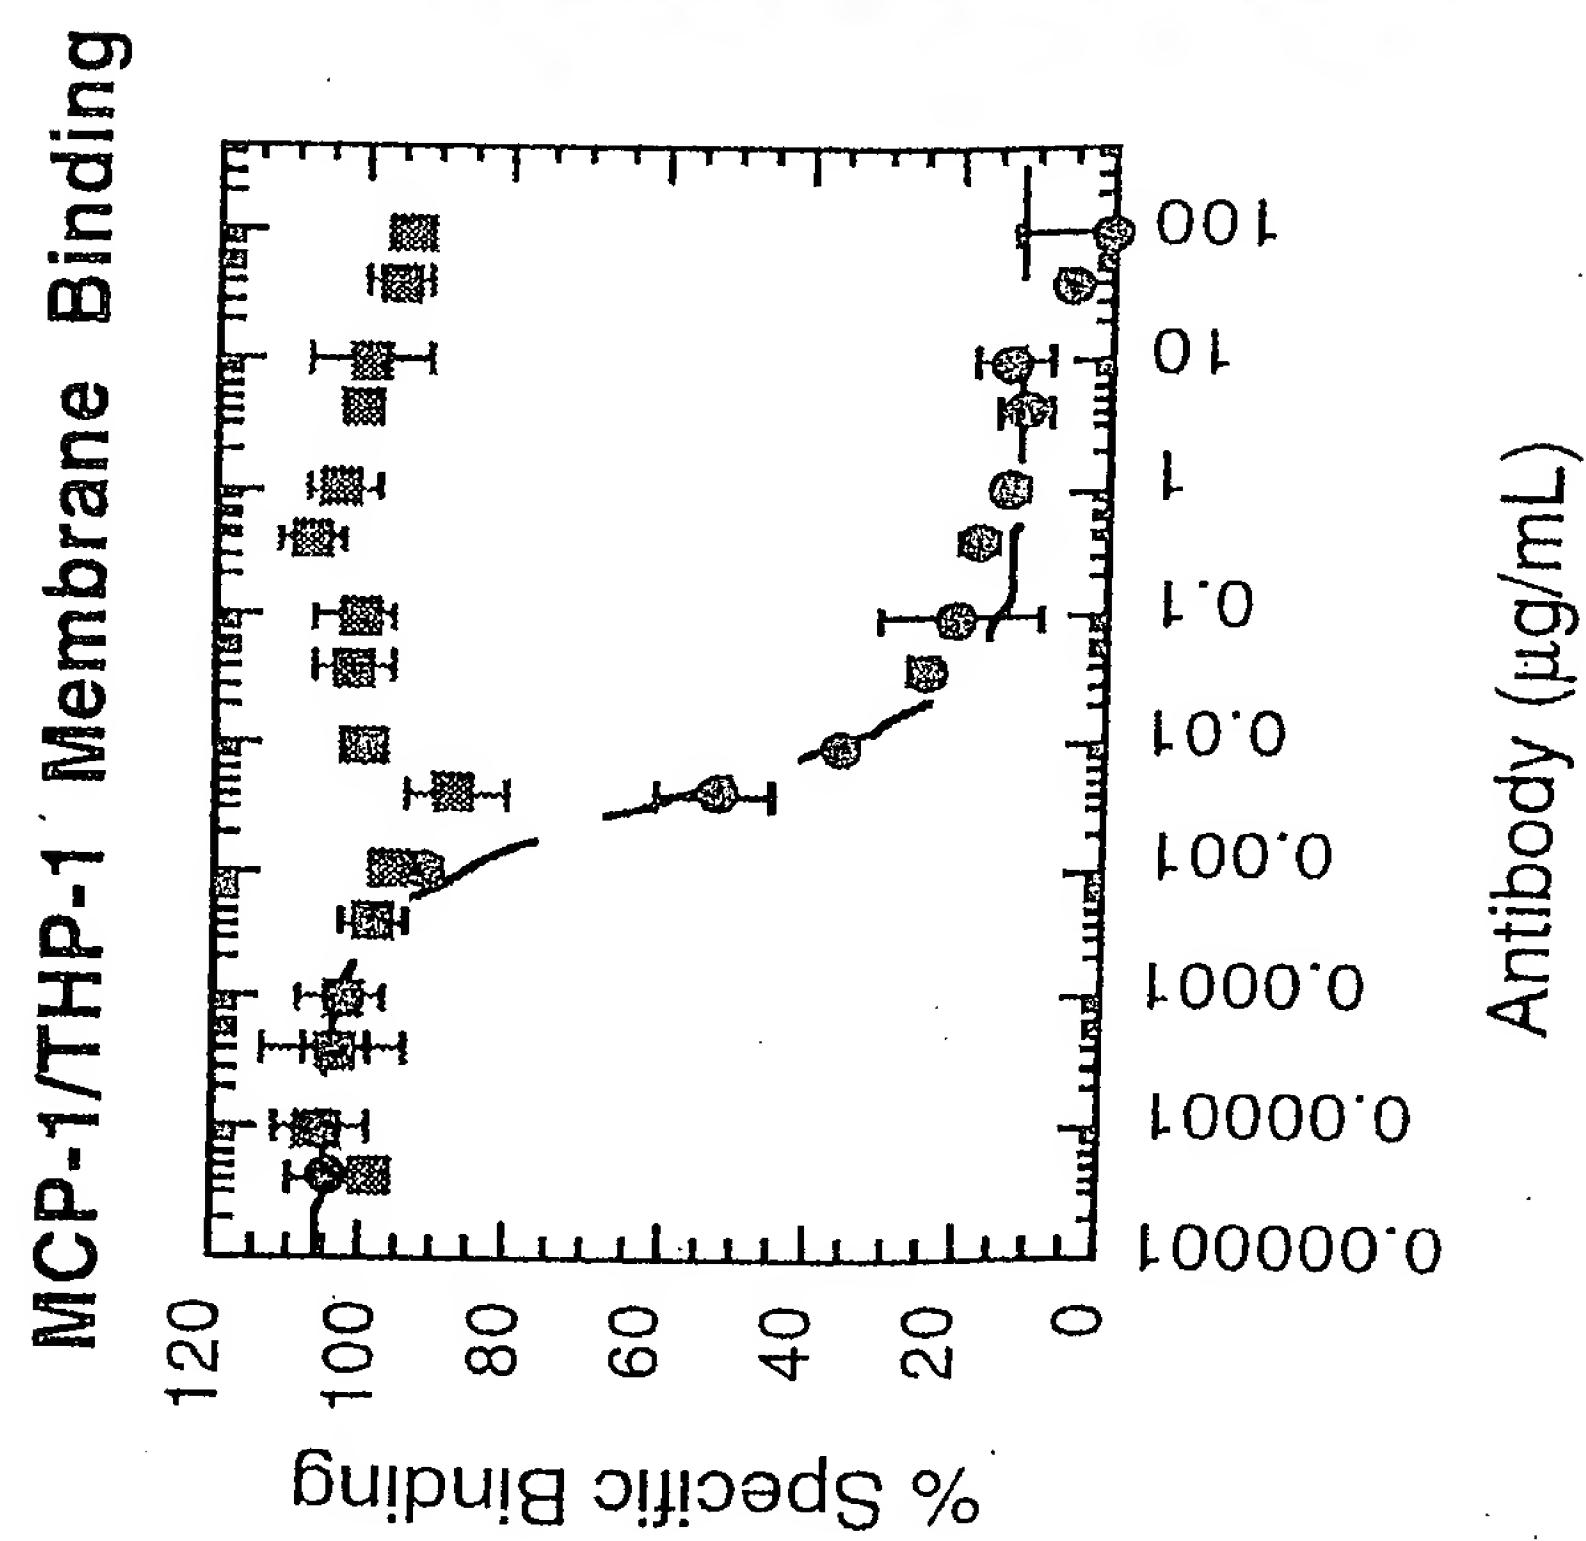

1D9 ($\mu\text{g/mL}$)		
	Value	Error
IC50	0.0037891	0.00062521
Hill	1.0185	0.15131
Bmax	105.63	2.6422
Bmin	11.518	1.9284
Chisq	280.01	NA
R	0.9948	NA

FIG. 4

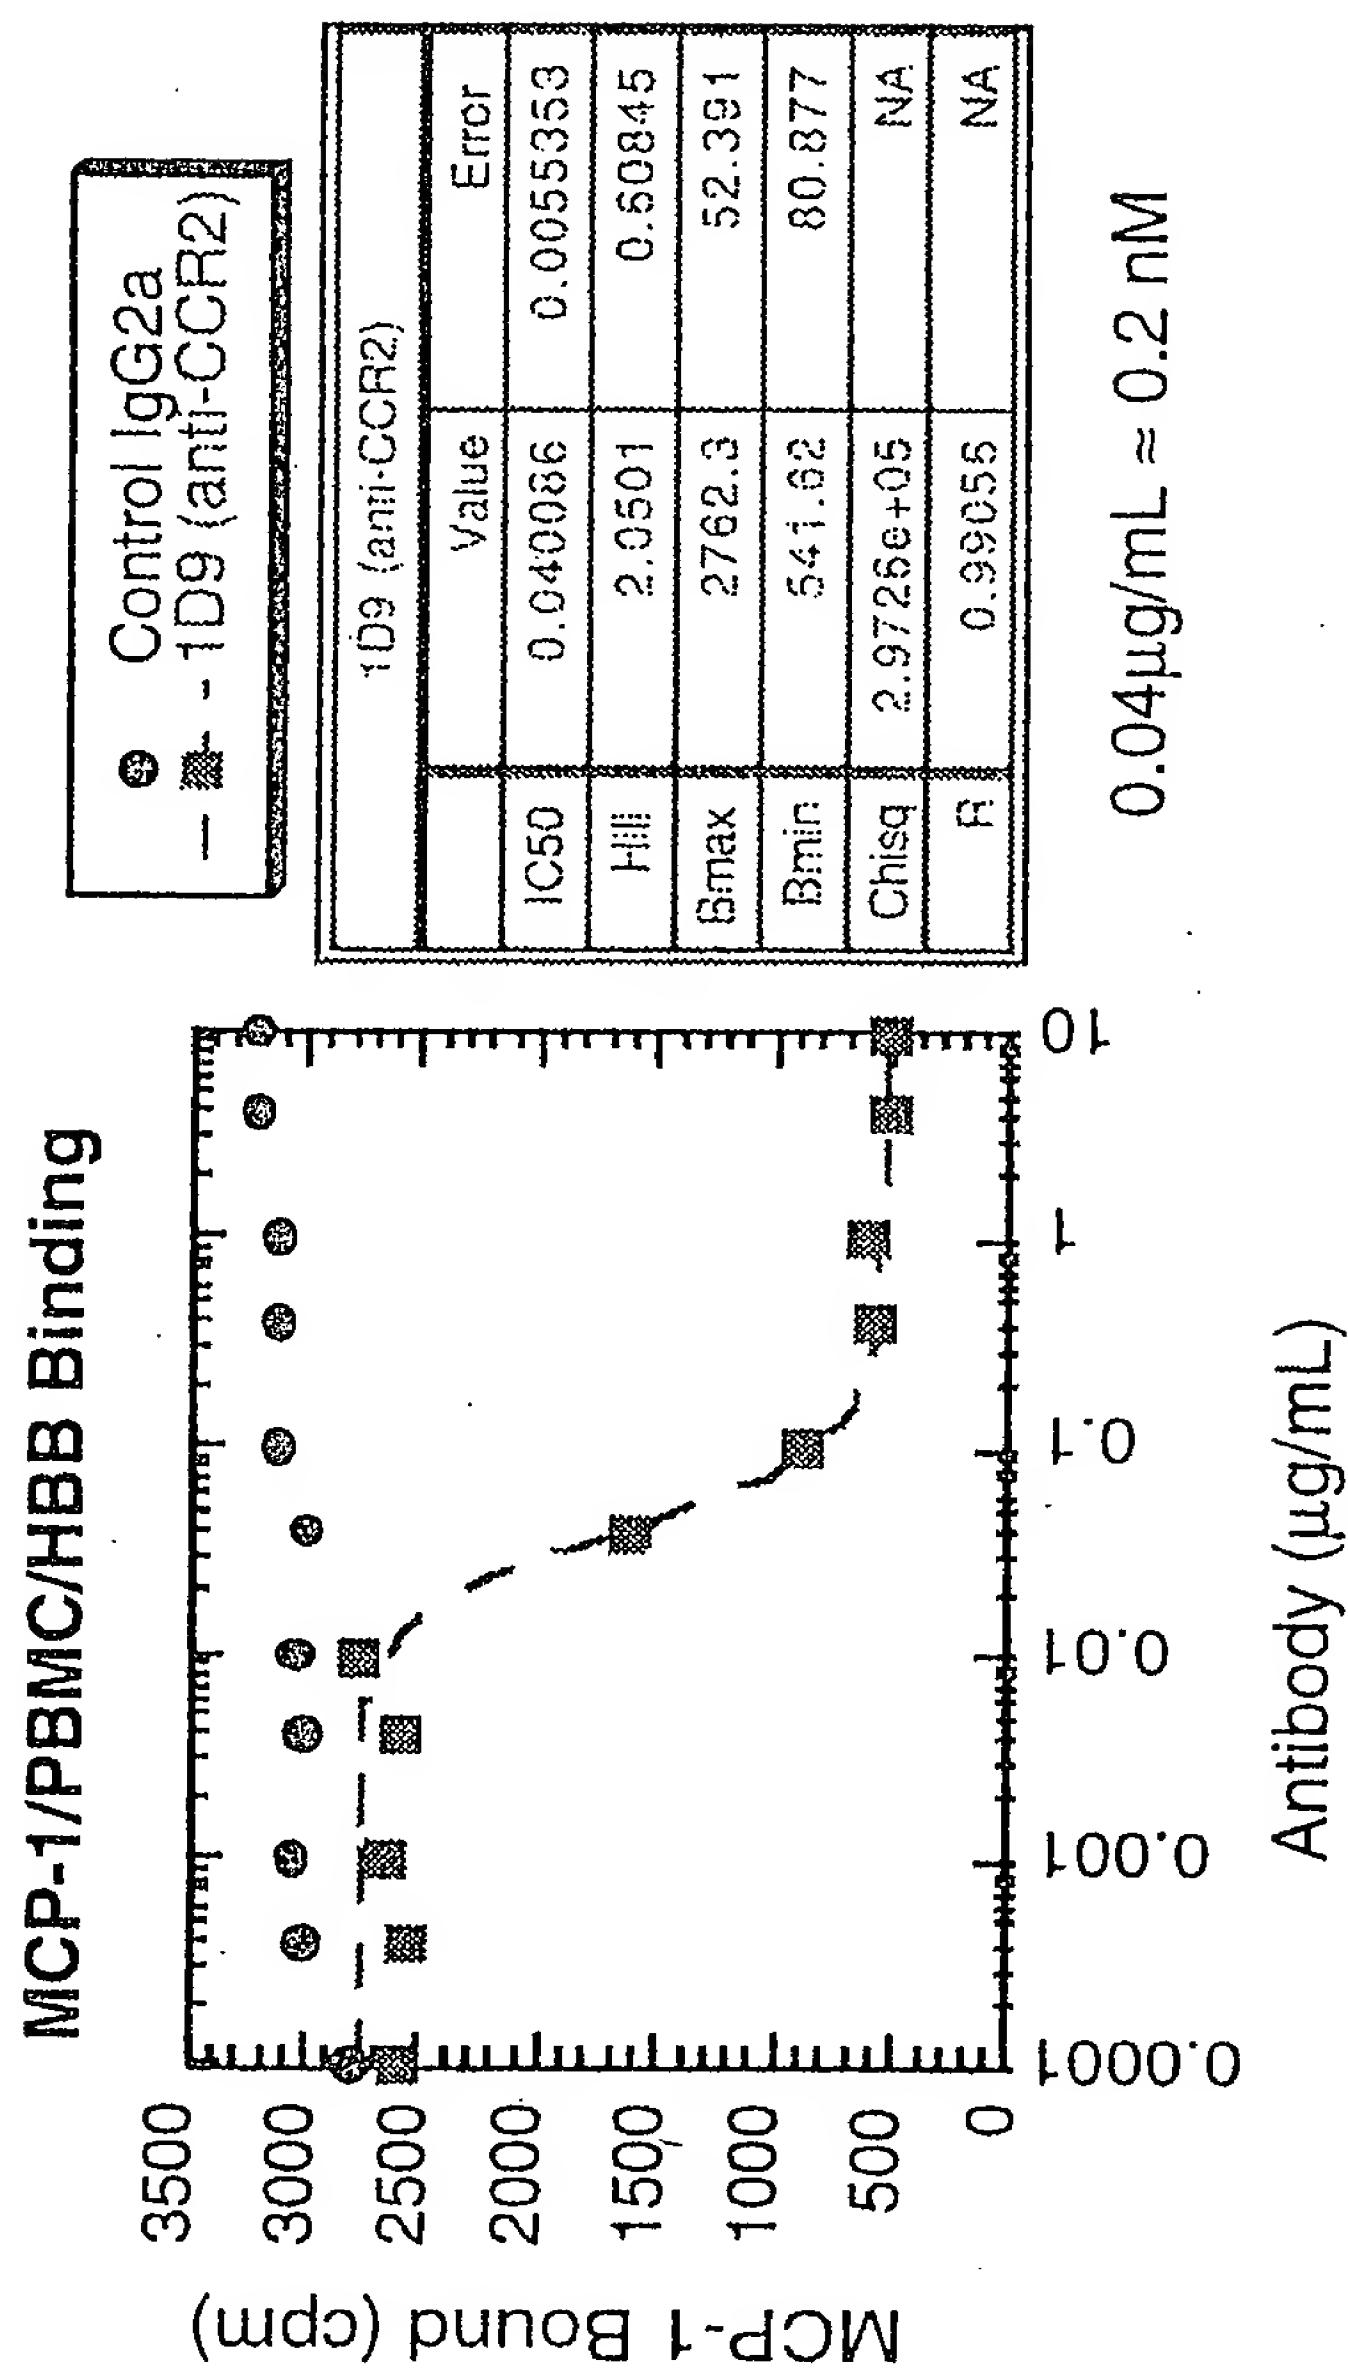


FIG. 5

Fig. 6B

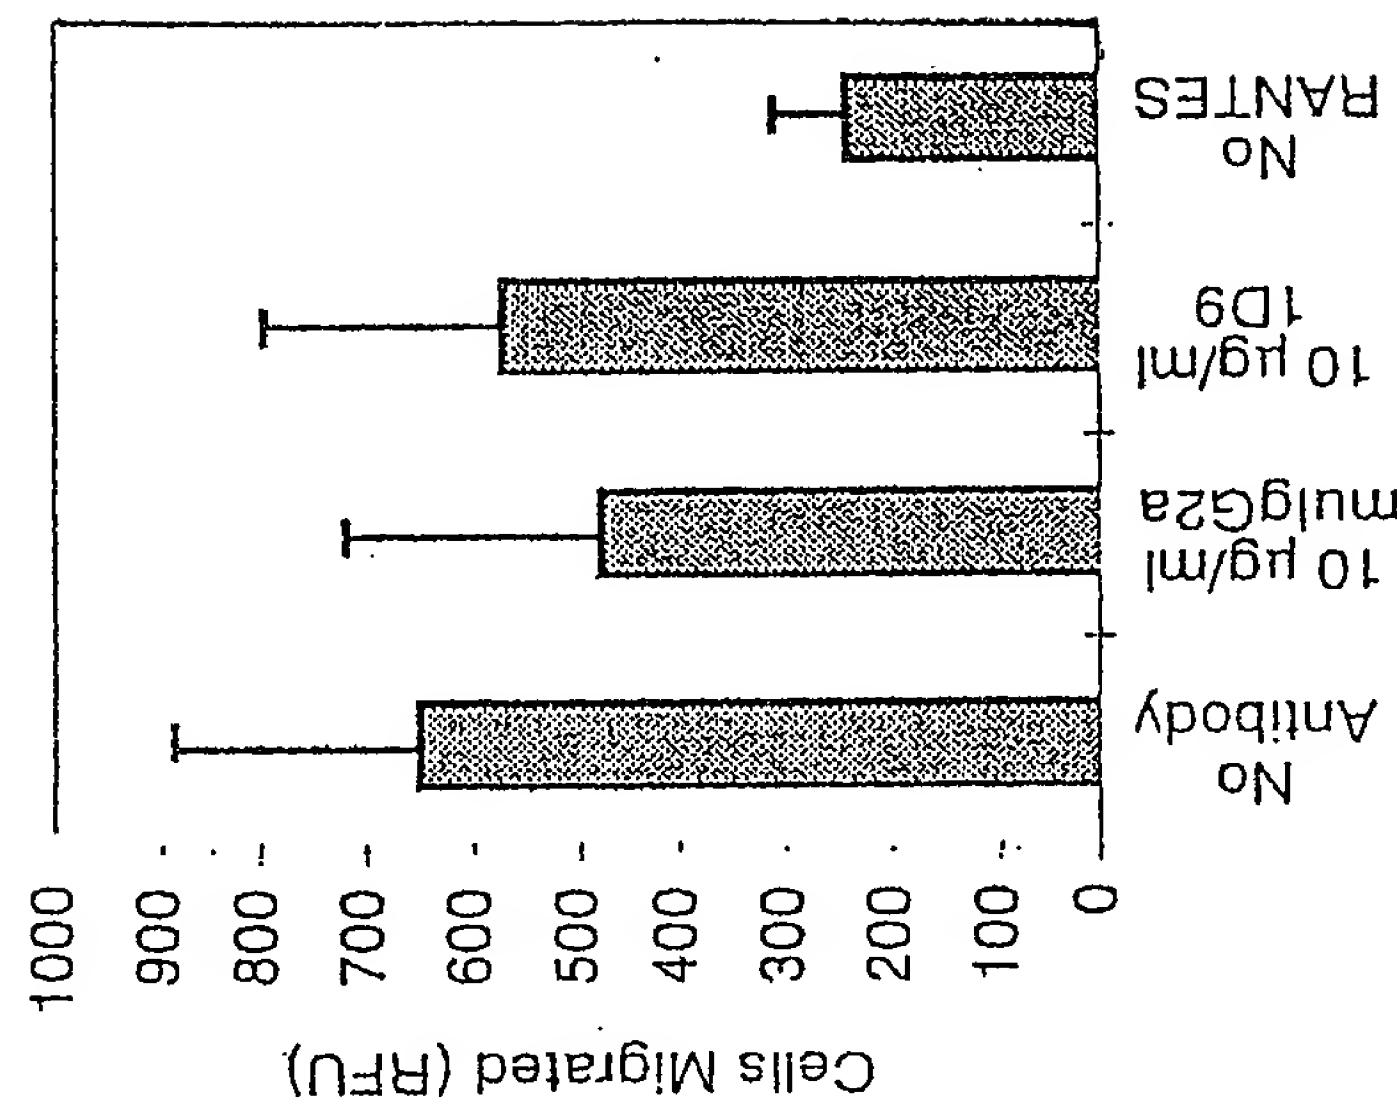


Fig. 6A

